

# **Purification of GST-tagged Proteins**

## **User Manual**

Protino® GST/4B Columns 1 ml

Protino® GST/4B Columns 5 ml

January 2010/Rev.01

## Table of contents

1	Components	4
1.1	Kit contents and storage	4
1.2	Reagents, consumables, and equipment to be supplied by the user	4
2	Introduction	6
2.1	Specifications	6
2.2	Culture size	7
2.3	Preparation of buffers	9
3	Safety instructions – risk and safety phrases	11
4	Protocols	12
4.1	Preparation of cleared <i>E. coli</i> lysates	12
4.2	Purification of GST-tagged proteins using Protino® GST/4B Columns	14
5	Regeneration and storage	16
6	Appendix	17
6.1	Troubleshooting	17
6.2	Ordering information	19
6.3	Product use restriction / warranty	20

# 1 Components

## 1.1 Kit contents and storage

Protino® GST/4B Columns			
	1 ml	5 ml	
<b>Cat. No.</b>	<b>745510.5</b>	<b>745515.1</b>	<b>745515.5</b>
Protino® GST/4B Columns	5 x 1 ml	1 x 5 ml	5 x 5 ml
User Manual	1	1	1

### Shipping and storage of Protino® GST/4B Columns:



The product is shipped at ambient temperature.

Upon receipt Protino® GST/4B Columns should be **stored at 4°C** and are stable up to 1 year. Do not freeze.

## 1.2 Reagents, consumables, and equipment to be supplied by the user

### Reagents

- PBS (10 mM Na<sub>2</sub>HPO<sub>4</sub>, 1.8 mM KH<sub>2</sub>PO<sub>4</sub>, 2.7 mM KCl, 140 mM NaCl, pH 7.3), see section 2.3
- Elution Buffer (50 mM Tris-HCl, 10 mM glutathione, pH 8), see section 2.3
- Lysozyme (required for cell extract preparation, see section 4.1)

### Consumables

- Appropriate centrifuge tubes, collecting tubes

### Equipment

- Appropriate centrifuge
- Liquid chromatography system (MPLC, FPLC™, ÄKTAdesign™, etc.), peristaltic pump, or syringe
- If necessary, appropriate adaptors for connecting the Protino® GST/4B Columns to your system of choice. Protino® GST/4B Columns are equipped with 10 – 32 (1/16") inlet and outlet ports. With these ports the columns can easily be connected to standard MPLC/FPLC™ systems, (e.g., ÄKTAdesign™). Five

adaptor sets are available for connecting the columns to other systems or for using them with a syringe (see Table 1).

**Table 1: Adaptor sets**

<b>System</b>	<b>Connec- tion via</b>	<b>Adaptor needed</b>	<b>Adaptor Set</b>
Standard FPLC™ system (e.g., ÄKTAdesign™)	10– 32	none	none
FPLC™ system, first generation (Pharmacia)	M6	1 x M6 female to 10– 32 male 1 x 10– 32 female to M6 male	Protino® M6 Adaptor Set Cat. No. 745260
MPLC system (e.g., BioLogic™, BIO-RAD)	1/4" 28	1 x 1/4" 28 female to 10– 32 male 1 x 10– 32 female to 1/4" 28 female	Protino® 1/4-28 Adaptor Set Cat. No. 745261
MPLC system (e.g., BioLogic™, BIO-RAD)	Luer	1 x Luer female to 10– 32 male 1 x 10– 32 female to Luer male	Protino® Luer Adaptor Set Cat. No. 745264
Peristaltic pump	1/16" ID tubing inlet	1 x 1/16" ID tubing to 10– 32 male	Protino® Inlet PP Adaptor Set Cat. No. 745263
Syringe	Luer inlet	1 x Luer female to 10– 32 male	Protino® Inlet Luer Adaptor Cat. No. 745262

## 2 Introduction

Protino® GST/4B Columns are convenient, ready-to-use FPLC™ columns prepacked with Protino® Glutathione Agarose 4B for rapid purification of GST fusion proteins. The columns can be used with an automated chromatography system, a peristaltic pump, or with a syringe for manual processing.

Protino® GST/4B Columns can be attached directly to liquid chromatography systems (such as ÄKTAdesign™ systems) via standard 10 – 32 fittings. The columns can also be operated with other chromatography systems, with a syringe, or peristaltic pump by using common adapters provided separately by MN (for details see section 1.2 or contact Technical Service Bioanalysis).

The snap-off end of the columns can be reused as stop plug for sealing the outlet of the columns for storage.

### 2.1 Specifications

**Table 2: Specifications Protino® GST/4B Columns**

Column bed volume	1 ml	5 ml
<b>System compatibility</b>	<ul style="list-style-type: none"> <li>- Automated liquid chromatography systems (MPLC, FPLC™, ÄKTAdesign™, etc.)</li> <li>- Peristaltic pump</li> <li>- Syringe</li> </ul>	
<b>Column dimensions</b>	0.7 cm inner diameter x 2.5 cm height	1.6 cm inner diameter x 2.5 cm height
<b>Column body material</b>	Polypropylene	
<b>Column ports</b>	Inlet 10 – 32 (1/16") female Outlet 10 – 32 (1/16") male	
<b>Matrix</b>	4% beaded agarose	
<b>Ligand</b>	Glutathione, linked via sulfur atom	
<b>Spacer arm</b>	12 atoms	
<b>Bead size</b>	90 µm	
<b>Binding capacity<sup>1</sup></b>	~10 mg (recombinant GST)	~50 mg (recombinant GST)

<sup>1</sup> Binding capacity will vary for each GST-tagged protein.

**Table 2: Specifications Protino® GST/4B Columns**

<b>Maximum back pressure</b>	3 bar (0.3 MPa)			
<b>Recommended flow rates</b>				
<b>Equilibration</b>	1.0	ml/min	2.5	ml/min
<b>Sample loading<sup>2</sup></b>	0.2 – 1.0 ml/min		0.5 – 2.0 ml/min	
<b>washing and elution</b>	1.0	ml/min	5.0	ml/min
<b>Chemical stability</b>	Protino® GST/4B Columns withstand incubation in 0.1 M acetate pH 4, 0.1 M NaOH, 70% ethanol, or 6 M guanidine hydrochloride for 2 hours at room temperature without significant loss of protein yield			
<b>Storage temperature</b>	4 – 8°C			
<b>Storage solution</b>	20% ethanol			


## 2.2 Culture size

The yield of GST-tagged proteins depends on various parameters, such as nature of the fusion protein, expression host, culture conditions, etc. However, some recommendations on protein load and culture size can be given (see Figure 1).

Culture volume requirements are based on the following assumptions:

- Protino® GST/4B Columns have a binding capacity of ~ 10 mg of recombinant GST per 1 ml bed volume.
- Typically, the expression level of GST-tagged proteins is high, ranging from 10 to 50 mg/liter of *E. coli* culture.
- As a starting point we recommend to use the cell lysate from a 200 – 1000 ml *E. coli* culture per 1 ml bed volume.

<sup>2</sup> Slow flow rates are recommended for the loading step to allow maximal binding of the GST-tagged protein .

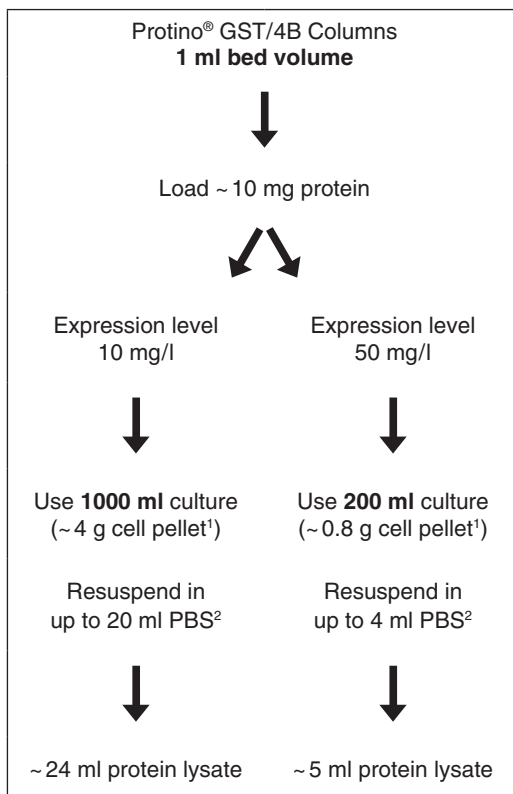

**Figure 1: Required culture volumes per 1 ml bed volume**

---

<sup>1</sup> On average, 250 ml of culture will produce approximately 1 g of pelleted, wet cells.

<sup>2</sup> 1 g cells may be lysed in 2 – 5 ml PBS, see section 4.1.

## 2.3 Preparation of buffers

### PBS (1 liter):

10 mM NaH <sub>2</sub> PO <sub>4</sub>	1.780 g Na <sub>2</sub> HPO <sub>4</sub> • 2 H <sub>2</sub> O	M <sub>r</sub> = 156.01 g/mol
1.8 mM KH <sub>2</sub> PO <sub>4</sub>	0.245 g KH <sub>2</sub> PO <sub>4</sub>	M <sub>r</sub> = 136.09 g/mol
2.7 mM KCl	0.201 g KCl	M <sub>r</sub> = 74.55 g/mol
140 mM NaCl	8.182 g NaCl	M <sub>r</sub> = 58.44 g/mol

Adjust pH to 7.3

### Elution Buffer (1 liter):

50 mM Tris base	6.06 g Tris base	M <sub>r</sub> = 121.14 g/mol
10 mM glutathione	3.07 g glutathione	M <sub>r</sub> = 307.3 g/mol

Adjust pH to 8.0

Prepare fresh daily and store at 4°C

Minimum buffer volumes required for one column run can be calculated according to the following table. Note that additional volumes of PBS and Elution Buffer may be prepared to flush lines and pumps depending on the chromatographic system. As a starting point we recommend to prepare approximately **150 ml of PBS** and **100 ml of Elution Buffer** for the 1 ml column and **300 ml of PBS** and **150 ml of Elution Buffer** for the 5 ml column. Use high-purity chemicals and water for preparing the buffers. For best results, filter buffers through a 0.45 µm filter before use.

### Protino® GST/4B Columns

1 ml	5 ml
------	------

### PBS

5 ml per 1 g of cell pellet for cell extract preparation	20 ml	100 ml
10 ml per 1 ml bed volume for equilibration	10 ml	50 ml
10 ml per 1 ml bed volume for washing	10 ml	50 ml
~50 ml of PBS for flushing lines and pump	50 ml	50 ml
Total volume of PBS	90 ml	250 ml
<b>Recommended volume of PBS</b>	<b>150 ml</b>	<b>300 ml</b>



**Protino® GST/4B Columns**

**1 ml**

**5 ml**

---

**Elution Buffer**

10 ml per 1 ml bed volume for equilibration                      10 ml                      50 ml

~50 ml of Elution Buffer for flushing lines and pump                      50 ml                      50 ml

Total volume of Elution Buffer                      60 ml                      100 ml

**Recommended volume of Elution Buffer                      100 ml                      150 ml**

---

### 3 Safety instructions – risk and safety phrases

The following components of the **Protino® GST/4B Columns** kits contain hazardous contents.

Component	Hazard contents	Hazard symbol	Risk phrases	Safety phrases
Protino® GST/4B Columns 1 ml and 5 ml	Ethanol 20%	*	Flammable R 10	

#### Risk phrases

R 10          Flammable

\* Hazard labeling not necessary if quantity per bottle below 125 g or ml (certificate of exemption according to 67/548/EEC Art. 25, 1999/45/EC Art. 12 and German GefStoffV § 20 (3) and TRGS 200 7.1). For further information see Material Safety Data Sheet.

## 4 Protocols

### 4.1 Preparation of cleared *E. coli* lysates



Refer to sections 2.2 for detailed information on culture volume requirements. Prepare PBS as described at section 2.3.

---

#### 1 Cultivate and harvest cells

- As a starting point we recommend to prepare 200 – 1000 ml *E. coli* expression culture for the purification of 10 mg of GST-tagged protein per 1 ml bed volume using Protino® GST/4B Columns (see section 2.2).
  - Harvest cells from an *E. coli* expression culture by centrifugation at 4,500 – 6,000 x *g* for 15 min at 4°C. Remove supernatant.
  - Cell pellets may be stored at -20°C or -80°C until needed.
- 

#### 2 Resuspend bacteria cells

- Thaw the cell pellet from an *E. coli* expression culture on ice (if frozen).
  - Resuspend 1 g of pelleted, wet cells in 2 – 5 ml PBS. Pipette up and down, or stir until complete resuspension without visible cell aggregates. Perform this step on ice.
- 

#### 3 Lyse cells

- Add lysozyme to a final concentration of 1 mg/ml.
  - Stir the solution on ice for 30 min.
  - Sonicate the suspension on ice according to the instructions provided by the manufacturer (e.g., use 10 x 15 s bursts with a 15 s cooling period between each burst).
  - Carefully check samples' appearance after sonication. If the lysate is still viscous from incomplete fragmentation of DNA, add 5 µg/ml DNase I and stir on ice for 15 min.
-

#### 4 Clarify lysate

- Centrifuge the crude lysate at 10,000 x *g* for 30 min at 4°C to remove cellular debris.
  - Carefully transfer the supernatant to a clean tube without disturbing the pellet. If the supernatant is not clear, centrifuge a second time or filter through a 0.45 µm membrane (e.g., cellulose acetate).
  - Store supernatant on ice.
- 

Proceed to section 4.2.

## 4.2 Purification of GST-tagged proteins using Protino® GST/4B Columns

Protino® GST/4B Columns can be operated with liquid chromatography systems (such as ÄKTAdesign™ systems) via standard 10 – 32 fittings without additional connectors.

Prepare buffers according to section 2.3. For best results, filter buffers through a 0.45 µm filter before use. Clear samples by centrifugation and/or pass them through a 0.45 µm filter.

Binding kinetics between GST and immobilized glutathione is relatively slow. Therefore use low flow rates for the loading step to allow maximal binding of the GST-tagged protein.

**!** Prepare Elution Buffer as described at section 2.3. Elution Buffer has to be prepared fresh daily and stored at 4°C.

### Protino® GST/4B Columns

1 ml

5 ml

#### 1 Connect column to the chromatography system

- Purge the pump with PBS. Assure that all air is displaced.
- Remove the snap-off end at the column outlet and save it for further use.
- Remove the upper plug from the column.
- Start the pump at a flow rate of approximately 0.3 ml/min.
- Fill the inlet port of the column with several drops of PBS to remove air to form a positive meniscus.
- Insert the fitting “drop-to-drop” into the column port to avoid introducing air bubbles.

*Note: The snap-off end can be reused as a stop plug for sealing the column outlet for storage.*

#### 2 Column equilibration

- Equilibrate the column with 5 – 10 column volumes of PBS until the baseline at 280 nm is stable.

5 – 10 ml

50 – 100 ml

Use a flow rate up to

1 ml/min

2.5 ml/min

## Protino® GST/4B Columns

1 ml

5 ml

**3 Binding**

- Load the centrifuged or filtered sample onto the column.
- Use a flow rate up to

0.2 – 1.0 ml/min

0.5 – 2 ml/min

*Note: Binding kinetics between GST and immobilized glutathione is relatively slow. Therefore use low flow rates for the loading step to allow maximal binding of the GST-tagged protein.*

- Collect flow through and analyze, for example by SDS-PAGE to verify that the GST-tagged protein has bound. If the fusion protein is found in early fractions of the flow-through, the flow rate should be decreased. If the fusion protein is absent in early fractions and does appear in late fractions of the flowthrough the column capacity has been exceeded. In this case protein load should be reduced or bed volume should be increased.

**4 Washing**

- Wash the column with 10 column volumes of PBS or until the baseline at 280 nm is stable.

10 ml

50 ml

Use a flow rate up to

1 ml/min

5 ml/min

**5 Elution**

- Elute the GST-tagged protein with 10 column volumes of Elution Buffer and collect fractions.

10 ml

50 ml

Use a flow rate up to

1 ml/min

5 ml/min

- Use a Bradford protein assay, SDS-PAGE, or measure the absorbance at 280 nm to identify the fraction(s) which contain(s) the majority of the eluted GST-tagged protein and analyze by SDS-PAGE.

## 5 Regeneration and storage

Reuse of Protino® GST/4B Columns should only be performed with identical GST-tagged proteins to avoid possible cross-contamination. The lifetime of the matrix depends on the nature of the sample.

If a single GST-tagged protein is to be purified several times, simply wash with 10 column volumes of PBS prior to the next column run.

**Basic cleaning:** Wash column with approximately 10 column volumes of 100 mM Tris-HCl + 0.5 M NaCl, pH 8.5, followed by approximately 10 column volumes of 100 mM sodium acetate + 0.5 M NaCl, pH 4.5. Repeat the above wash cycles twice. Wash with 5 column volumes of PBS.

**Rigorous cleaning:** To remove precipitated or denatured proteins wash with 2 column volumes of 6 M guanidine hydrochloride, immediately followed by 5 – 10 column volumes of PBS. To remove hydrophobically bound contaminants, wash with 4 column volumes of 70% ethanol or 1% Triton X-100 followed by 5 – 10 column volumes of PBS.

If you will not be using the matrix immediately wash with additional 5 column volumes of 20% ethanol and store at 4°C.

## 6 Appendix

### 6.1 Troubleshooting

Problem	Possible cause and suggestions
Low protein yield	<p><i>Problems with vector construction</i></p> <ul style="list-style-type: none"> <li>• Ensure that protein and tag are in frame.</li> </ul>
	<p><i>Low protein expression</i></p> <ul style="list-style-type: none"> <li>• Optimize bacterial expression conditions.</li> </ul>
	<p><i>Fusion protein forms insoluble aggregates (inclusion bodies)</i></p> <ul style="list-style-type: none"> <li>• Lower the growth temperature from 37°C to 30 – 15°C.</li> </ul>
Fusion protein does not bind efficiently	<p><i>Extraction may be insufficient</i></p> <ul style="list-style-type: none"> <li>• Check extraction conditions (lysozyme, sonication).</li> <li>• Use up to 2% of a non-ionic detergent to improve cell disruption and/or solubilization of the fusion protein.</li> </ul>
	<p><i>Sonication may have been too severe</i></p> <ul style="list-style-type: none"> <li>• Choose milder sonication conditions. Over-sonication can alter the conformation of the GST moiety and prevents the fusion protein from binding to Protino® GST/4B Columns.</li> </ul>
	<p><i>Reducing agent missing</i></p> <ul style="list-style-type: none"> <li>• Adding DTT to the lysis buffer (final concentration 5 mM) prior to cell lysis can significantly increase binding of some fusion proteins.</li> </ul>
	<p><i>Flow rate too high</i></p> <ul style="list-style-type: none"> <li>• Decrease flow rate for the loading step to allow maximal binding of the GST-tagged protein.</li> </ul>
	<p><i>Concentration of fusion protein is too dilute</i></p> <ul style="list-style-type: none"> <li>• Concentrate the sample. Yield depends on the concentration of the fusion protein in the lysate. If the sample is too dilute, fusion proteins may not bind efficiently.</li> </ul>



Problem	Possible cause and suggestions
Fusion protein does not bind efficiently <i>(continued)</i>	<p data-bbox="309 213 885 234"><i>Protino® GST/4B Columns have been used several times</i></p> <ul data-bbox="309 245 984 347" style="list-style-type: none"> <li data-bbox="309 245 984 347">• Clean matrix according to section 5 or use fresh matrix. Immobilized glutathione can be degraded by <math>\gamma</math>-glutamyl transpeptidase activity in <i>E. coli</i> cell lysates. Therefore, matrices with immobilized glutathione have a finite lifetime.</li> </ul>
Fusion protein elutes inefficiently	<p data-bbox="309 392 505 413"><i>Low elution volume</i></p> <ul data-bbox="309 424 984 501" style="list-style-type: none"> <li data-bbox="309 424 984 501">• Increase the volume of Elution Buffer. Depending on the nature of the fusion protein and the amount of protein loaded, additional elution steps or buffer volume is required.</li> </ul> <p data-bbox="309 544 491 564"><i>Flow rate too high</i></p> <ul data-bbox="309 576 684 596" style="list-style-type: none"> <li data-bbox="309 576 684 596">• Decrease flow rate during elution.</li> </ul> <p data-bbox="309 639 589 660"><i>Incorrect buffer composition</i></p> <ul data-bbox="309 671 984 748" style="list-style-type: none"> <li data-bbox="309 671 984 748">• Check composition and pH of the Elution Buffer. In some cases up to 50 mM reduced glutathione may be used to improve elution.</li> </ul> <p data-bbox="309 791 822 812"><i>Elution Buffer not prepared immediately before use</i></p> <ul data-bbox="309 823 818 844" style="list-style-type: none"> <li data-bbox="309 823 818 844">• Prepare Elution Buffer immediately before use.</li> </ul>
Poor protein purity	<p data-bbox="309 887 510 908"><i>Insufficient washing</i></p> <ul data-bbox="309 919 768 940" style="list-style-type: none"> <li data-bbox="309 919 768 940">• Increase the number of washes with PBS.</li> </ul> <p data-bbox="309 983 656 1003"><i>Degradation of GST fusion protein</i></p> <ul data-bbox="309 1015 984 1091" style="list-style-type: none"> <li data-bbox="309 1015 984 1091">• Add a protease inhibitor to the lysis solution. Multiple bands may be the result of partial degradation by host proteases during the purification procedure.</li> </ul> <ul data-bbox="309 1118 984 1235" style="list-style-type: none"> <li data-bbox="309 1118 984 1166">• Keep all samples and buffers on ice to reduce the activity of proteases.</li> <li data-bbox="309 1182 984 1235">• Use a protease-deficient host. Multiple bands may be the result of partial degradation by host proteases during cell growth.</li> </ul> <p data-bbox="309 1278 689 1299"><i>Sonication may have been too severe</i></p> <ul data-bbox="309 1310 984 1390" style="list-style-type: none"> <li data-bbox="309 1310 984 1390">• Choose milder sonication conditions. Over-sonication can lead to the co-purification of host proteins with the GST-tagged protein.</li> </ul>

---

**Problem**                      **Possible cause and suggestions**


---

Poor protein purity (continued)	<i>Co-purification of chaperonins</i>
	<ul style="list-style-type: none"> <li>Several chaperonins, that are involved in protein folding, may co-purify with GST fusion proteins, for example DnaK (~ 70 kDa), DnaJ (~ 37 kDa), GrpE (~ 40 kDa), GroEL (~ 57 kDa), GrpE (~ 40 kDa), GroEL (57 kDa), GroES (~ 10 kDa). Several additional purification steps have been described. For example co-purification of DnaK can be avoided by treating the cell lysate with 5 mM MgCl<sub>2</sub> and 5 mM ATP prior to purification. DnaK can be dissociated from other components in the presence of ATP and Mg<sup>2+</sup>.</li> </ul>

---

## 6.2 Ordering information

Product	Cat. No.	Pack of
Protino® GST/4B Columns 1 ml	745510.5	5 columns
Protino® GST/4B Columns 5 ml	745515.1 745515.5	1 column 5 columns
Protino® Glutathione Agarose 4B	745500.10	10 ml (settled agarose beads)
	745500.100	100 ml (settled agarose beads)
Protino® M6 Adaptor Set	745260	1 set
Protino® 1/4-28 Adaptor Set	745261	1 set
Protino® Luer Adaptor Set	745264	1 set
Protino® Inlet PP Adaptor Set	745263	1 set
Protino® Inlet Luer Adaptor	745262	1

Visit [www.mn-net.com](http://www.mn-net.com) for more detailed product information.

### 6.3 Product use restriction / warranty

**Protino® GST/4B Columns** were developed, designed, distributed, and sold **FOR RESEARCH PURPOSES ONLY**. They are suitable **FOR IN-VITRO USES ONLY**. No claim or representation is intended for its use to identify any specific organism or for clinical use (diagnostic, prognostic, therapeutic, or blood banking).

It is rather the responsibility of the user to verify the use of the **Protino® GST/4B Columns** for a specific application range as the performance characteristic of this kit has not been verified to a specific organism.

This MACHEREY-NAGEL product is shipped with documentation stating specifications and other technical information. MACHEREY-NAGEL warrants to meet the stated specifications. MACHEREY-NAGEL's sole obligation and the customer's sole remedy is limited to replacement of products free of charge in the event products fail to perform as warranted. Supplementary reference is made to the general business terms and conditions of MACHEREY-NAGEL, which are printed on the price list. Please contact us if you wish an extra copy.

MACHEREY-NAGEL does not warrant against damages or defects arising in shipping and handling (transport insurance for customers excluded), or out of accident or improper or abnormal use of this product; against defects in products or components not manufactured by MACHEREY-NAGEL, or against damages resulting from such non-MACHEREY-NAGEL components or products.

MACHEREY-NAGEL makes no other warranty of any kind whatsoever, and SPECIFICALLY DISCLAIMS AND EXCLUDES ALL OTHER WARRANTIES OF ANY KIND OR NATURE WHATSOEVER, DIRECTLY OR INDIRECTLY, EXPRESS OR IMPLIED, INCLUDING, WITHOUT LIMITATION, AS TO THE SUITABILITY, REPRODUCTIVITY, DURABILITY, FITNESS FOR A PARTICULAR PURPOSE OR USE, MERCHANTABILITY, CONDITION, OR ANY OTHER MATTER WITH RESPECT TO MACHEREY-NAGEL PRODUCTS.

In no event shall MACHEREY-NAGEL be liable for claims for any other damages, whether direct, indirect, incidental, compensatory, foreseeable, consequential, or special (including but not limited to loss of use, revenue or profit), whether based upon warranty, contract, tort (including negligence) or strict liability arising in connection with the sale or the failure of MACHEREY-NAGEL products to perform in accordance with the stated specifications. This warranty is exclusive and MACHEREY-NAGEL makes no other warranty expressed or implied.

The warranty provided herein and the data, specifications and descriptions of this MACHEREY-NAGEL product appearing in MACHEREY-NAGEL published catalogues and product literature are MACHEREY-NAGEL's sole representations concerning the product and warranty. No other statements or representations, written or oral, by MACHEREY-NAGEL's employees, agent or representatives, except written statements signed by a duly authorized officer of MACHEREY-NAGEL are authorized; they should not be relied upon by the customer and are not a part of the contract of sale or of this warranty.

Product claims are subject to change. Therefore please contact our Technical Service Team for the most up-to-date information on MACHEREY-NAGEL products. You may also contact your local distributor for general scientific information. Applications mentioned in MACHEREY-NAGEL literature are provided for informational purposes only. MACHEREY-NAGEL does not warrant that all applications have been tested in MACHEREY-NAGEL laboratories using MACHEREY-NAGEL products. MACHEREY-NAGEL does not warrant the correctness of any of those applications.

Please contact:  
MACHEREY-NAGEL Germany  
Tel.: +49 (0) 24 21 969 270  
e-mail: TECH-BIO@mn-net.com

Last updated: 12/2006, Rev.02

---

**Trademarks:**

ÄKTAdesig and FPLC are trademarks of GE Healthcare companies  
BioLogic and Profinia are trademarks of BIO-RAD Laboratories, Inc.  
Protino is a registered trademark of MACHEREY-NAGEL

All used names and denotations can be brands, trademarks, or registered labels of their respective owner – also if they are not special denotation. To mention products and brands is only a kind of information (i.e., it does not offend against trademarks and brands and can not be seen as a kind of recommendation or assessment). Regarding these products or services we can not grant any guarantees regarding selection, efficiency, or operation.